



BROMINE KIT

OCTA-SLIDE 2, 0.2-3.0 ppm


CODE 6955-01

QUANTITY	CONTENTS	CODE
50	Bromine Tablets	6977A-H
2	Test Tubes, plastic, 2.5-5-10mL, w/caps	0106
1	Octa-Slide 2 Viewer	1101
1	Bromine Octa-Slide 2 Bar, 0.2-3.0 ppm	6822-01

*WARNING: Reagents marked with an * are considered to be potential health hazards. To view or print a Material Safety Data Sheet (MSDS) for these reagents go to www.lamotte.com. To obtain a printed copy, contact LaMotte by e-mail, phone or fax.

To order individual reagents or test kit components, use the specified code number.

USE OF THE OCTA-SLIDE 2 VIEWER

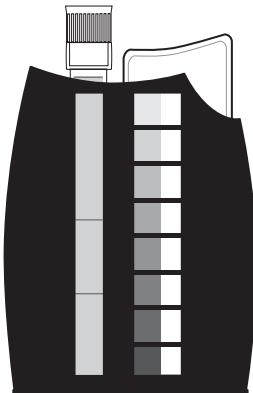

The Octa-Slide 2 Viewer should be held so non-direct light enters through the back of the Viewer. Slide the Octa-Slide 2 Bar into the Viewer. Insert the reacted sample into the top of the Viewer. Match the color of the reaction to the color standards.

WARNING! This set contains chemicals that may be harmful if misused. Read cautions on individual containers carefully. Not to be used by children except under adult supervision.

PROCEDURES

A diagram showing a vertical white slide with a grey scale on the left being lowered into a black rectangular viewer.	<p>1</p> <p>Insert Bromine Octa-Slide 2 Bar (6822-01) into the Octa-Slide 2 Viewer (1101).</p>
A diagram showing a vertical test tube being filled with a grey liquid from the bottom.	<p>2</p> <p>Fill a test tube (0106) to the 5 mL line with the water sample.</p>
A diagram showing a small white tablet being dropped into a vertical test tube.	<p>3</p> <p>Add one Bromine Tablet (6977A).</p>
A diagram showing a vertical test tube with a grey liquid being capped and then rotated with circular arrows at both ends.	<p>4</p> <p>Cap and mix until tablet disintegrates.</p>
A diagram showing a vertical test tube with a grey liquid being inserted into a black rectangular viewer.	<p>5</p> <p>Insert test tube into Octa-Slide 2 Viewer.</p>
A diagram showing the black rectangular viewer with the test tube inserted, which is then shown inserted into a larger black slide viewer.	<p>6</p> <p>Match sample color to a color standard. Record as ppm Bromine.</p>

NOTE: Thoroughly clean and rinse test tubes after each use.

LaMOTTE COMPANY

Helping People Solve Analytical Challenges

PO Box 329 · Chestertown · Maryland · 21620 · USA
800-344-3100 · 410-778-3100 [Outside U.S.A.] · Fax 410-778-6394
Visit us on the web at www.lamotte.com